



## ZytoDot 2C SPEC 19q13/19p13 Probe

<b>REF</b> C-3037-100	$\nabla$	10 (0.1 ml)
<b>REF</b> C-3037-400	$\nabla$	40 (0.4 ml)

For the qualitative detection of the human chromosome 19q13.32-q13.33 deletions and 19p13.3 specific sequences by chromogenic *in situ* hybridization (CISH)



In vitro diagnostic medical device  
according to EU directive 98/79/EC

### 1. Intended use

The ZytoDot 2C SPEC 19q13/19p13 Probe (PD22) is intended to be used for the qualitative detection of human 19q13.32-q13.33 deletions and the detection of 19p13.3 specific sequences in formalin-fixed, paraffin-embedded specimens by chromogenic *in situ* hybridization (CISH). The probe is intended to be used in combination with the ZytoDot 2C CISH Implementation Kit (Prod. No. C-3044-10/-40).

Interpretation of the results must be made within the context of the patient's clinical history with respect to further clinical and pathologic data of the patient by a qualified pathologist.

### 2. Clinical relevance

Deletions affecting the short arm of chromosome 1 (1p) are frequently found in human gliomas and neuroblastomas, but also in breast, lung, endometrial, ovarian, and colorectal carcinomas. Deletions affecting the long arm of chromosome 19 (19q) are frequently found in human malignant gliomas as well as in neuroblastomas and epithelial ovarian cancers. Combined loss of the complete 1p/19q chromosome arms, caused by an unbalanced t(1;19)(q10;p10) translocation, is characteristic of oligodendrogliomas. According to the 2016 WHO criteria for classification of tumors of the central nervous system, the detection of 1p/19q loss is required for the diagnosis of WHO grade II or III "oligodendroglioma, IDH-mutant and 1p/19q codeleted". Since both, astrocytomas and oligodendrogliomas, can exhibit IDH mutations, evaluation of 1p/19q status plays a critical role in differentiating astrocytoma from oligodendroglioma. Oligodendroglioma morphology, IDH-mutant genotype, and 1p/19q codeletion are associated with better response to chemotherapy and improved survival. Hence, determination of 1p and 19q status may aid in therapeutic decisions and predict outcome in patients with diffuse gliomas.

### 3. Test principle

The chromogenic *in situ* hybridization (CISH) technique allows the detection and visualization of specific nucleic acid sequences in cell preparations. Hapten-labeled nucleotide fragments, so called CISH probes, and their complementary target sequences in the preparations are co-denatured and subsequently allowed to anneal during hybridization.

Afterwards, unspecific and unbound probe fragments are removed by stringency washing steps. Duplex formation of the labeled probe can be visualized using primary (unmarked) antibodies, which are detected by secondary polymerized enzyme-conjugated antibodies. The enzymatic reaction with chromogenic substrates leads to the formation of colored precipitates. After counterstaining the nucleus with a nuclear dye, hybridized probe fragments are visualized by light microscopy.

### 4. Reagents provided

The ZytoDot 2C SPEC 19q13/19p13 Probe is composed of:

- Dinitrophenyl-labeled polynucleotides (~0.8 ng/ $\mu$ l), which target sequences mapping in 19q13.32-q13.33\* (chr19:47,857,776-48,339,398) (see Fig. 1).
- Digoxigenin-labeled polynucleotides (~0.8 ng/ $\mu$ l), which target sequences mapping in 19p13.3\* (chr19:815,938-962,244) (see Fig. 1).
- Formamide based hybridization buffer

\*according to Human Genome Assembly GRCh37/hg19

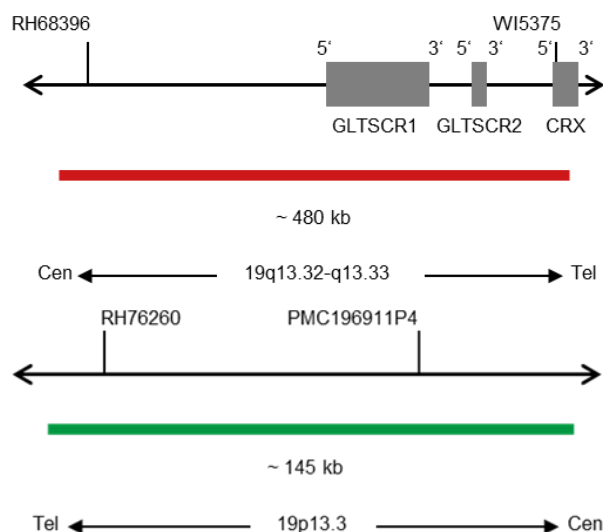


Fig. 1: Top: SPEC 19q13 Probe map; Bottom: SPEC 19p13 Probe map (not to scale)

The ZytoDot 2C SPEC 19q13/19p13 Probe is available in two sizes:

- C-3037-100: 0.1 ml (10 reactions of 10  $\mu$ l each)
- C-3037-400: 0.4 ml (40 reactions of 10  $\mu$ l each)

### 5. Materials required but not provided

- ZytoDot 2C CISH Implementation Kit (Prod. No. C-3044-10/-40)
- Positive and negative control specimens
- Microscope slides, positively charged
- Water bath (80°C, 98°C)
- Hybridizer or hot plate
- Hybridizer or humidity chamber in hybridization oven
- Adjustable pipettes (10  $\mu$ l, 1000  $\mu$ l)
- Staining jars or baths
- Timer
- Calibrated thermometer
- Ethanol or reagent alcohol
- Xylene
- Methanol 100%
- Hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>) 30%
- Deionized or distilled water
- Coverslips (22 mm x 22 mm, 24 mm x 32 mm)
- Rubber cement, e.g., Fixogum Rubber Cement (Prod. No. E-4005-50/-125) or similar
- Adequately maintained light microscope (400-630x)

## 6. Storage and handling

Store at 2-8°C in an upright position. Return to storage conditions immediately after use. Do not use reagents beyond expiry date indicated on the label. The product is stable until expiry date indicated on the label when handled accordingly.

## 7. Warnings and precautions

- Read the instructions for use prior to use!
- Do not use the reagents after the expiry date has been reached!
- This product contains substances (in low concentrations and volumes) that are harmful to health and potentially infectious. Avoid any direct contact with the reagents. Take appropriate protective measures (use disposable gloves, protective glasses, and lab garments)!
- Report any serious incident that has occurred in relation to the product to the manufacturer and the competent authority according to local regulations!
- If reagents come into contact with skin, rinse skin immediately with copious amounts of water!
- A material safety data sheet is available on our homepage ([www.zytovision.com](http://www.zytovision.com)).
- Do not reuse reagents, unless reuse is explicitly permitted!
- Avoid any cross-contamination and micro-bacterial contamination of the reagents!
- The specimens must not be allowed to dry during the hybridization and washing steps!

### Hazard and precautionary statements:

The hazard-determining component is formamide.



### Danger

H351	Suspected of causing cancer.
H360FD	May damage fertility. May damage the unborn child.
H373	May cause damage to organs through prolonged or repeated exposure.
P201	Obtain special instructions before use.
P202	Do not handle until all safety precautions have been read and understood.
P260	Do not breathe dust/fume/gas/mist/vapours/spray.
P280	Wear protective gloves/protective clothing/eye protection/face protection.
P308+P313	IF exposed or concerned: Get medical advice/attention.
P405	Store locked up.

## 8. Limitations

- For *in vitro* diagnostic use.
- For professional use only.
- For non-automated use only.
- The clinical interpretation of any positive staining, or its absence, must be done within the context of clinical history, morphology, other histopathological criteria as well as other diagnostic tests. It is the responsibility of a qualified pathologist to be familiar with the CISH probes, reagents, diagnostic panels, and methods used to produce the stained preparation. Staining must be performed in a certified, licensed laboratory under the supervision of a pathologist who is responsible for reviewing the stained slides and assuring the adequacy of positive and negative controls.
- Specimen staining, especially signal intensity and background staining, is dependent on the handling and processing of the specimen prior to staining. Improper fixation, freezing, thawing, washing, drying, heating, sectioning, or contamination with other specimens or fluids may produce artefacts or false results. Inconsistent results may result from variations in fixation and embedding methods, as well as from inherent irregularities within the specimen.

- The probe should be used only for detecting loci described in chapter 4. "Reagents provided".
- The performance was validated using the procedures described in these instructions for use. Modifications to these procedures might alter the performance and have to be validated by the user.

## 9. Interfering substances

The following fixatives are incompatible with ISH:

- Bouin's fixative
- B5 fixative
- Acidic fixatives (e.g., picric acid)
- Zenker's fixative
- Alcohols (when used alone)
- Mercuric chloride
- Formaldehyde/zinc fixative
- Hollande's fixative
- Non-buffered formalin

## 10. Preparation of specimens

Recommendations:

- Avoid cross-contamination of samples in any step of preparation as this may lead to erroneous results.
- Fixation in 10% neutrally buffered formalin for 24 h at room temperature (18-25°C).
- Sample size  $\leq 0.5 \text{ cm}^3$ .
- Use premium quality paraffin.
- Embedding should be carried out at temperatures lower than 65°C.
- Prepare 3-5  $\mu\text{m}$  microtome sections.
- Use positively charged microscope slides.
- Fix tissue sections for 2-16 h at 50-60°C.

## 11. Preparatory treatment of the device

The product is ready-to-use. No reconstitution, mixing, or dilution is required. Bring probe to room temperature (18-25°C) and mix briefly before use.

## 12. Assay procedure

### Specimen pretreatment

Perform specimen pretreatment (e.g., dewaxing, proteolysis) according to the instructions for use of the ZytoDot 2C CISH Implementation Kit.

### Denaturation and hybridization

1. Pipette 10  $\mu\text{l}$  of the probe onto each pretreated specimen.
2. Cover specimens with a 22 mm x 22 mm coverslip (avoid trapped bubbles) and seal the coverslip.

*We recommend using rubber cement (e.g., Fixogum) for sealing.*

3. Place slides on a hot plate or hybridizer and denature specimens for 5 min at 79°C.
4. Transfer slides to a humidity chamber and hybridize overnight at 37°C (e.g., in a hybridization oven).

*It is essential that specimens do not dry out during the hybridization step.*

### Post-hybridization

Perform post-hybridization processing (washing, detection, counter-staining, mounting, microscopy) according to the instructions for use of the ZytoDot 2C CISH Implementation Kit.

## 13. Interpretation of results

Using the ZytoDot 2C CISH Implementation Kit, hybridization signals of Digoxigenin-labeled polynucleotides appear as dark green colored distinct dots (19p13 locus), and Dinitrophenyl-labeled polynucleotides appear as bright red colored distinct dots (19q13 locus).

**Normal situation:** In interphases of normal cells or cells without deletion involving the 19q13 locus, two distinct dot-shaped red and two distinct dot-shaped green signals appear (see Fig. 2).

**Aberrant situation:** In a cell with deletion affecting the 19q13 locus, a reduced number of red signals will be observed. Deletions affecting only parts of the 19q13 locus might result in a normal signal pattern with red signals of reduced size (see Fig. 2).

Overlapping signals may appear as brown signals.

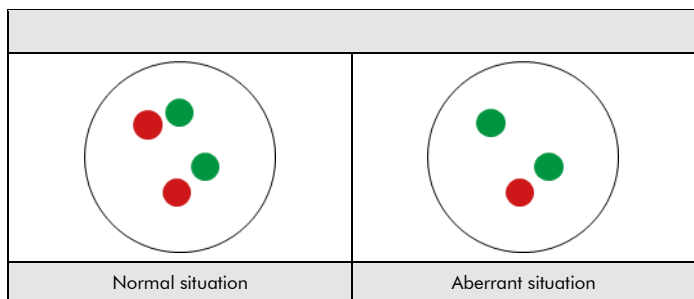


Fig. 2: Expected results in normal and aberrant nuclei

Other signal patterns than those described above may be observed in some abnormal samples. These unexpected signal patterns should be further investigated.

**Please note:**

- Due to decondensed chromatin, single CISH signals can appear as small signal clusters. Thus, two or three signals of the same size, separated by a distance  $\leq 1$  signal diameter, should be counted as one signal.
- Prior to signal enumeration, the specimen should be scanned for any possible intratumoral heterogeneity at 100- to 200-fold magnification.
- Visualization of signals should be performed at least at 400-fold magnification resulting in easily visible signals. A 630-fold magnification is recommended for probes detecting chromosomal breaks. Do not use contrast enhancing filter lenses as this might distort the signal color. To obtain signals in bright colors, open the aperture diaphragm. Be sure to focus up and down when evaluating a nucleus, as red and green signals might be located on top of each other.
- Do not evaluate areas of necrosis, overlapping nuclei, over-digested nuclei and nuclei with weak signal intensity.
- Due to mitosis, additional signals may be visible even in a small percentage of non-neoplastic cells. Occasionally, nuclei with missing signals may be observed in paraffin-embedded specimens due to cutting artefacts.
- A negative or unspecific result can be caused by multiple factors (see chapter 17. "Troubleshooting").
- In order to correctly interpret the results, the user must validate this product prior to use in diagnostic procedures according to national and/or international guidelines.

**14. Recommended quality control procedures**

In order to monitor correct performance of processed specimens and test reagents, each assay should be accompanied by internal and external controls. If internal and/or external controls fail to demonstrate appropriate staining, results with patient specimens must be considered invalid.

**Internal control:** Non-neoplastic cells within the specimen that exhibit normal signal pattern, e.g., fibroblasts.

**External control:** Validated positive and negative control specimens.

**15. Performance characteristics**

The performance of the probe was determined by comparison against the corresponding IVD approved FISH probe. The concordance was 100%.

**Accuracy:** The accuracy was calculated as 100%.

**Analytical sensitivity:** The analytical sensitivity was calculated as 100%.

**Analytical specificity:** The analytical specificity was calculated as 100%.

**16. Disposal**

The disposal of reagents must be carried out in accordance with local regulations.

**17. Troubleshooting**

Any deviation from the operating instructions can lead to inferior staining results or to no staining at all.

**Weak signals or no signals at all**

Possible cause	Action
Cell or tissue sample has not been properly fixed	Optimize fixing time and fixative
Heat pretreatment, proteolysis, hybridization, denaturation, stringency wash or antibody-incubation temperature not correct	Check temperature of all technical devices used, using a calibrated thermometer. Use always the same number of slides in solutions with critical temperature
Proteolytic pretreatment not carried out properly	Depending on multiple factors, e.g., nature and duration of fixing, thickness of sections, and nature of tissue/cells, different incubation times may be required. Ascertain the optimum time for pepsin incubation in pre-tests
Hybridization time too short	Hybridize for at least 12 h; extend hybridization time if necessary
Old dehydration solutions	Prepare fresh dehydration solutions
Probe evaporation	When using a hybridizer, the use of the wet stripes/water filled tanks is mandatory. When using a hybridization oven, the use of a humidity chamber is required. In addition, the coverslip should be sealed completely, e.g., with Fixogum, to prevent drying-out of the sample during hybridization
Incubation with chromogenic substrate too short	Extend incubation time
Counterstaining time too long	The counterstaining time depends on the nature of the specimen and should be optimized accordingly. Avoid dark counterstaining, because it may obscure positive staining signals
Bluing of counterstain not carried out properly	Use cold running tap water for bluing; do not use warm or hot water, or bluing reagents

**Signals too strong**

Possible cause	Action
Proteolytic pretreatment carried out too long	Depending on multiple factors, e.g., nature and duration of fixing, thickness of sections, and nature of tissue/cells, different incubation times may be required. Ascertain the optimum time for pepsin incubation in pre-tests
AP-Red Solution incubation time not correct	If required, the incubation time can be shortened down to 5 min. Do not heat substrate solution over 25°C; incubate at room temperature only
HRP-Green solution incubation time not correct	If required, the incubation time can be shortened down to 7 min. Do not heat substrate solution over 25°C; incubate at room temperature only

**Red signals too weak**

Possible cause	Action
AP-Red Solution was exposed to strong direct light	Prepare and use AP-Red Solution protected from strong direct light
AP-Red Solution was prepared too early	Prepare prior to immediate use
AP-Red Solution incubation time not correct	If required, the incubation time can be extended up to 15 min
Insufficient preparation of chromogenic substrate	Do not increase volume of Solution A

**Green signals too weak**

Possible cause	Action
Incubation time of any washing steps after staining with HRP-Green too long	Do not exceed given incubation times
HRP-Green solution incubation time not correct	If required, the incubation time can be extended up to 15 min
Insufficient preparation of chromogenic substrate	Do not increase volume of Solution A

**Signals fade or merge**

Possible cause	Action
An unsuitable mounting solution has been used	Use only the mounting solution provided with the kit or xylene-based mounting solutions free of any impurities; do not use coverslip tape
Sections were not dehydrated properly	Use fresh ethanol and xylene solutions; use only xylene of "pure" quality

**Uneven or in some parts only very light staining**

Possible cause	Action
Incomplete dewaxing	Use fresh solutions; check duration of dewaxing times
Reagent volume too small	Ensure that the reagent volume is large enough to cover the tissue area
Air bubbles caught before hybridization or during mounting	Avoid air bubbles

**Inconsistent results**

Possible cause	Action
Insufficient drying before probe application	Extend air-drying
Too much water/wash buffer on tissue prior to application of pepsin, antibodies and/or color substrates	Ensure that excess liquid is removed from tissue section by blotting or shaking it off the slide. Small amounts of residual water/wash buffer do not interfere with the test
Variations in tissue fixation and embedding methods	Optimize fixation and embedding methods
Variations in tissue section thickness	Optimize sectioning

**Morphology degraded**

Possible cause	Action
Cell or tissue sample has not been properly fixed	Optimize fixing time and fixative
Proteolytic pretreatment not carried out properly	Optimize pepsin incubation time; decrease if necessary

**Cross hybridization signals; noisy background**

Possible cause	Action
Stringency wash temperature not correct	Check temperature of the technical devices used, using a calibrated thermometer. Use always the same number of slides in the jar. We recommend not to use more than eight slides per jar for heat incubation steps
Slides not thoroughly rinsed	Use fresh and sufficient wash buffer and deionized or distilled water where indicated
Sections dried out any time during or after hybridization	Avoid sections being dried out; use humidity chamber; seal coverslip properly

Prolonged substrate incubation time	Shorten substrate incubation time
Incomplete dewaxing	Use fresh solutions; check duration of dewaxing
Proteolytic pretreatment too strong	Optimize pepsin incubation time
Slides cooled to room temperature before hybridization	Transfer the slides quickly to hybridization temperature

**Overlapping signals**

Possible cause	Action
Inappropriate thickness of tissue sections	Prepare 3-5 µm microtome sections

**Specimen floats off the slide**

Possible cause	Action
Unsuitable slide coating	Use appropriate (positively charged) slides
Proteolytic pretreatment too strong	Shorten pepsin incubation time

**18. Literature**

- Barbashina V, et al. (2005) *Clin Cancer Res* 11: 1119-28.
- Cairncross JG, et al. (1998) *J Natl Cancer Inst* 90: 1473-9.
- Cairncross G, et al. (2013) *J Clin Oncol* 31: 337-43.
- Caron H, et al. (1996) *N Engl J Med* 334: 225-30.
- Griffin CA, et al. (2006) *J Neuropathol Exp Neurol* 65: 988-94.
- Louis DN, et al. (ed.) (2016) *WHO Classification of Tumours of the Central Nervous System* (Revised 4th Edition).
- Lass U, et al. (2013) *Brain Pathol* 23: 311-8.
- Ragnarsson G, et al. (1999) *Br J Cancer* 79: 1468-74.
- Reifenberger G, et al. (2017) *Nat Rev Clin Oncol* 14: 434-52.
- Rosenberg JE, et al. (1996) *Oncogene* 13: 2483-5.
- Smith JS, et al. (1999) *Oncogene* 18: 4144-52.
- Smith JS, et al. (2000) *Genes Chromosomes Cancer* 29: 16-25.
- Wilkinson DG: *In Situ Hybridization, A Practical Approach*, Oxford University Press (1992) ISBN 0 19 963327 4.

**19. Revision**

Please refer to [www.zytovision.com](http://www.zytovision.com) for the most recent instructions for use as well as for instructions for use in different languages.

Our experts are available to answer your questions. Please contact [help@zytovision.com](mailto:help@zytovision.com)



ZytoVision GmbH  
Fischkai 1  
27572 Bremerhaven/ Germany  
Phone: +49 471 4832-300  
Fax: +49 471 4832-509  
[www.zytovision.com](http://www.zytovision.com)  
Email: [info@zytovision.com](mailto:info@zytovision.com)

**Trademarks:**

ZytoVision® and ZytoDot® are trademarks of ZytoVision GmbH.